

# High Speed, High Accuracy Tester Installation, Operation and Maintenance



Made in the  
United States of America



Figure 1. Vermason [222562](#) High Speed, High Accuracy Wrist Strap Tester

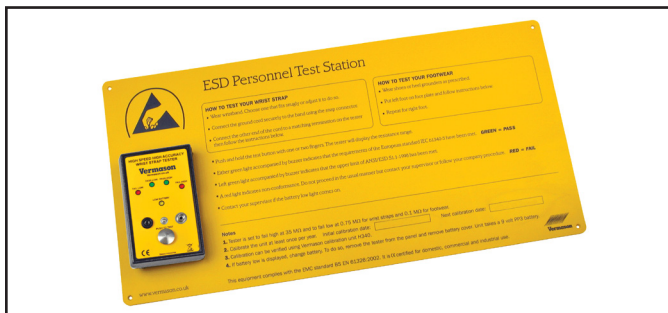


Figure 2. Vermason [222563](#) High Speed, High Accuracy Wrist Strap Test Station



Figure 3. Vermason [222564](#) High Speed, High Accuracy Wrist Strap / Footwear Test Station



Figure 4. Vermason [222565](#) High Speed, High Accuracy Wrist Strap / Footwear Test Station with Output

## Description

All models of the Vermason High Speed, High Accuracy Tester range comprise a digital test unit controlled by a programmable IC. They can test the efficiency of personnel grounding systems while being worn, by measuring the resistance in the circuit including the body of the operator. The instrument will indicate whether the resistance is in the ranges specified in EN 61340-5-1 using Annex A test method A.1.

“All personnel shall be grounded or equipotentially bonded ... when handling ESDs [ESD sensitive items]. When personnel are seated at ESD protective workstations, they shall be connected to ground via a wrist strap system” (EN 61340-5-1 clause 5.3.3 Personnel grounding)

“While wearing the wrist strap, connect the loose end of the cord to the tester terminal and depress the test button or touch the metal test surface with a finger or hand. If the resistance is over  $3,5 \times 10^7 \Omega$ , test the cord alone for continuity. If the resistance of the cord alone is approximately  $1,0 \times 10^6 \Omega$ , check the fit of the band around the wrist and adjust it for a snug fit. Snap the cord back on the cuff and retest. If the resistance is still over  $3,5 \times 10^7 \Omega$ , substitute a new band.” (CLC TR 61340-5-2 User guide Wrist Strap clause 4.7.2.4.3 Test procedure)

## Wrist Strap Test Frequency

“Wrist straps should be tested periodically. The frequency of testing, however, is driven by the amount of usage, wear and ESD risk exposure that can occur between tests. For, example, what is the quantity of product handled between test periods?

Typical test programs recommend that wrist straps that are used daily should be tested daily. However, if the products that are being produced are of such value that a guarantee of a continuous, reliable ground is needed then continuous monitoring should be considered or even required.” (CLC/TR 61340-5-2 User guide Wrist Strap clause 4.7.2.4.4 Test frequency)

NOTE 1: Electrical breakages within the cord can be checked by flexing the cord during measurement.

If the resistance is still too high, dry skin might be the problem. Dry skin conditions can be resolved by applying moisturising lotion on the wrist and repeating the resistance test again. The moisturising lotion should be one that is compatible with process requirements and does not cause contamination.

NOTE 2: Metal expansion bracelet style wristbands may trap moisture underneath and can be more effective for people with dry skin. (CLC/TR 61340-5-2 User guide Wrist Strap clause 4.7.2.4.3 Test procedure)

The Vermason High Speed, High Accuracy Tester is available in four models:

Item	Description
<a href="#">222562</a>	Wrist Strap Tester
<a href="#">222563</a>	Wrist Strap Test Station
<a href="#">222564</a>	Wrist Strap / Footwear Test Station
<a href="#">222565</a>	Wrist Strap / Footwear Test Station with Output

## Packaging

### Item [222562](#)

- 1 High Speed, High Accuracy Wrist Strap Tester
- 1 9 V Alkaline Battery

### Item [222563](#)

- 1 High Speed, High Accuracy Wrist Strap Tester
- 1 Wall Plate
- 1 9 V Alkaline Battery

### Item [222564](#)

- 1 High Speed, High Accuracy Wrist Strap / Footwear Tester
- 1 Wall Plate
- 1 Foot Plate, Single Foot
- 1 9 V Alkaline Battery

### Item [222565](#)

- 1 High Speed, High Accuracy Wrist Strap / Footwear Tester
- 1 Wall Plate
- 1 Foot Plate, Single Foot
- 1 Output Cable
- 1 9 V Alkaline Battery

## Installation

1. Insert the 9 V battery into the tester.
2. If applicable, install the tester at the desired location using the four mounting holes in the corners of the yellow wall plate.

3. If applicable, set the foot plate below the tester.
4. If applicable, connect the footwear lead at the bottom of the tester to the foot plate.

## [222565](#) WRIST STRAP / FOOTWEAR TEST STATION WITH OUTPUT

The [222565](#) tester features a relay terminal that can be integrated with electronic door locks, lights, buzzers, etc. It is capable of switching up to 0.5 A @ 50 VDC.

An Output Cable with stripped ends is included with the tester to help you wire your device to the tester's relay terminal. The list below describes the relay contacts for each wire.

White Wire = Normally Closed  
 Black Wire = Normally Open  
 Red Wire = Common

## Operation

### WRIST STRAP

1. Snap the coiled cord to the wristband and fit it snugly onto the wrist.
2. Connect the other end of the wrist cord to a matching termination on the tester.
3. Push and hold the test button until a result is displayed.

A green LED with buzzer indicates a PASS condition. A red LED indicates a FAIL condition.

Replace battery if the LOW BATTERY LED illuminates.

### FOOTWEAR

1. ESD Footwear covers heel grounders, toe grounders and ESD shoes/boots.
2. Place one foot on the foot plate and raise the other off the floor.
3. Push and hold the test button until a result is displayed.

A green LED with buzzer indicates a PASS condition. A red LED indicates a FAIL condition.

Replace battery if the LOW BATTERY LED illuminates.

4. Repeat Steps 2-3 for the other foot.

## Calibration

A periodic check (once every 6 to 12 months) using a precision resistance box should be performed to verify proper operation.

The Vermason [222547](#) Calibration Unit is available for the periodic testing of the High Speed, High Accuracy Testers.

The Calibration Unit can be used in the test location within a few minutes virtually eliminating downtime, verifying that the High Speed, High Accuracy Tester is operating within tolerances.

See [TB-7581](#) for more information.



Figure 5. Vermason [222547](#) Calibration Unit

## Specifications

Wrist Strap Limit	750 kilohm - 35 megohm
Footwear Limit	750 kilohm - 35 megohm
Accuracy	±10 %
Test Voltage	24 VDC
Dimensions	Tester 146 mm x 91 mm x 33 mm Wall Plate 300 mm x 600 mm x 3 mm Foot Plate 420 mm x 220 mm x 3 mm
Weight	0.3 kg (including battery and wall plate)
Power Supply	9 V battery or one of the following power adapters: <a href="#">19262</a>
Battery Life	approximately 3,000 tests (3 seconds per test)

## Limited Warranty, Warranty Exclusions, Limit of Liability and RMA Request Instructions

See the Desco Europe Warranty - [DescoEurope.com/Limited-Warranty.aspx](http://DescoEurope.com/Limited-Warranty.aspx)